

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
 Location: WEST WINDSOR POLICE
 Calibration File No.: 00984
 Certification File No.: 00985
 Linearity File No.: 00986
 Solution File No.: 01007
 Sequential File No.: 01007

Serial No.: ARWF-0382
 Calib. Date: 02/26/2013
 Cert. Date: 02/26/2013
 Lin. Date: 02/26/2013
 Soln. Date: 05/02/2013
 File Date: 05/02/2013
 Calib. No.: 00029
 Cert. No.: 00017
 Lin. No.: 00017
 Soln. No.: 00135

Calibrating Unit: WET
 Control Solution %: 0.100%
 Solution Control Lot: 12C100

Model No.: CU-34
 Serial No.: DDWJ S3-0363
 Expires: 03/02/2014
 Bottle No.: 0779

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:45D		
Control 1 EC	-.---%	10:46D	34.0°C	
Control 1 IR	-.---%	10:46D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		CTRL GAS SUPPLY
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCMAHON

First Name: MICHAEL

MI: J

Signature: _____

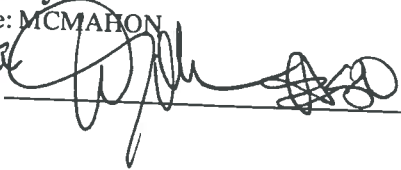

Badge No.: 80

Date: 05/02/2013